

# TEXIO

## 取扱説明書

ラックマウントフレーム

# RM-608J/E

株式会社 テクシオ・テクノロジー  
© PRINTED IN JAPAN B71-0033-00


ラックマウントフレーム RM-608J/E は、当社電源製品をJIS規格または EIA 規格の標準ラックにマウントするためのフレームです。

製品の取付には機器により別売りの取付金具をお求めください。

### 1. 構成部品リスト

		数量	備考
①	取手フレーム(R)	1 個	
②	取手フレーム(L)	1 個	
③	フレーム(棚板)	1 個	
④	フレーム(上)	1 個	* RM-608Jのみ
⑤	丸皿ネジ	4 個	N33-5014-41
⑥	山形ワッシャ	4 個	N19-0722-05
⑦	皿ネジ	10 個	N32-3006-41

### 2. ラックマウントフレーム組立方法

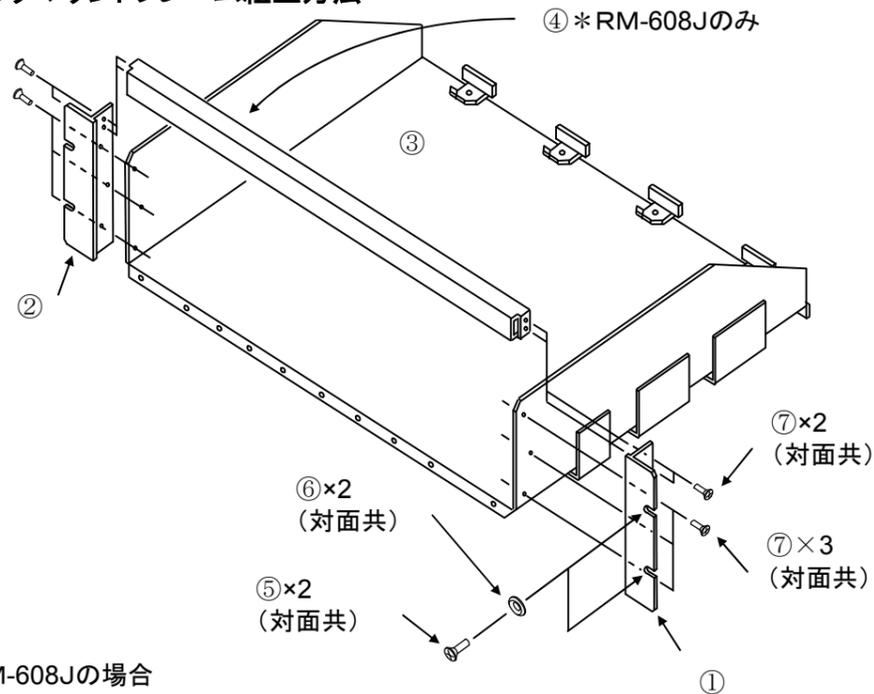

### 3. 機器組み込み手順



(1) 組立てたラックマウントフレームに、取付準備をした収納する機器を載せてください。

収納機器の背面側取付金具の凹部が、フレーム(棚板)③背面側の凸部にはまるまで、そのまま後方へ機器をスライドさせてください。

次に収納機器の前面側取付金具を、フレーム(棚板)③にセムスネジにて固定します(ネジは取付金具についているものをお使いください)。


(2) RM-608Jの場合

固定した収納機器の上側にフレーム(上)④を載せ、両側の取手フレーム(R)(L)へ皿ネジ⑦を使用し取付けます。

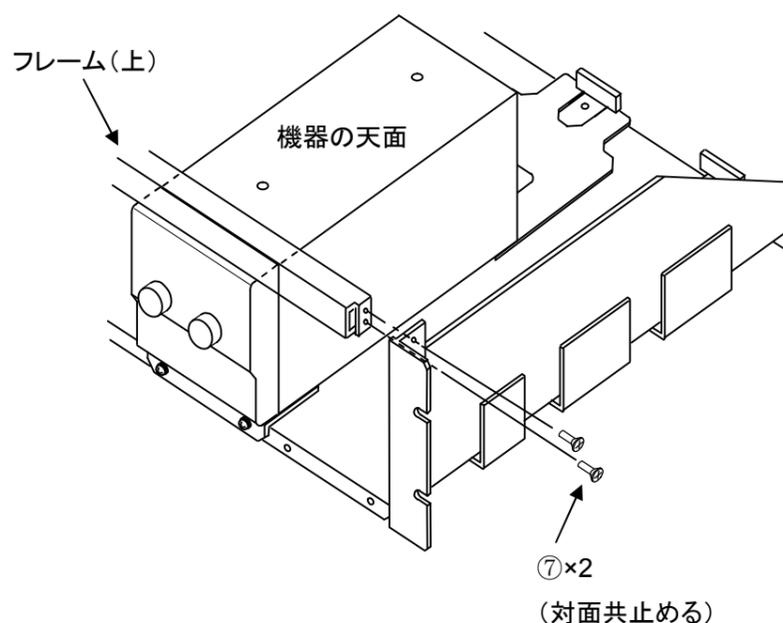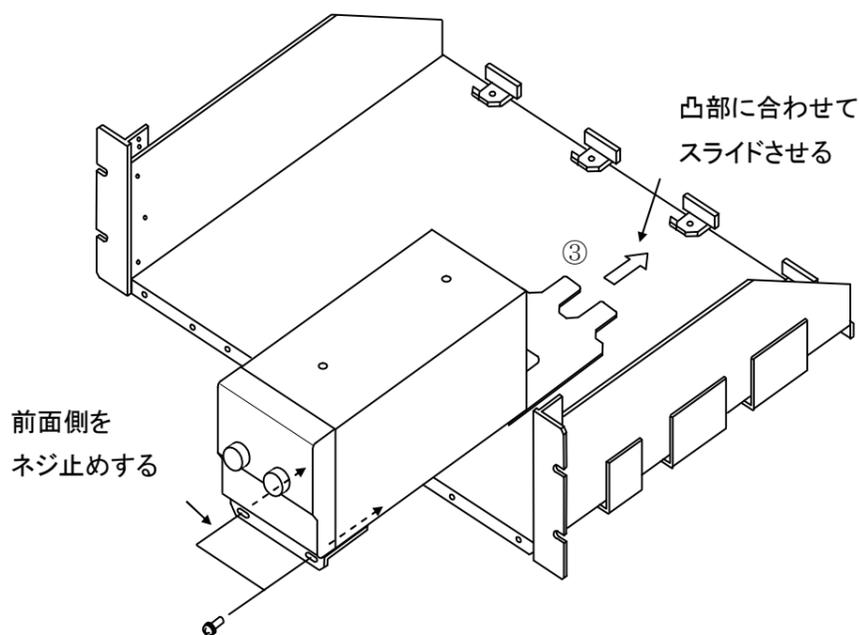

#### 注意事項

○ 重量物ですので、ラックに収納後はサポートアングルを取付けてください。

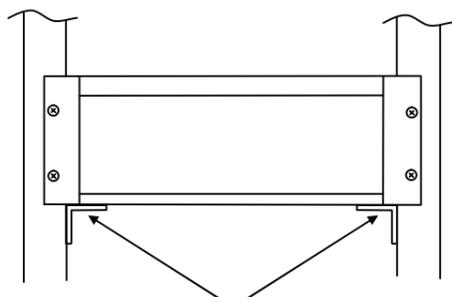

\* 当社ではサポートアングルを用意しておりません。  
市販のラックを使用されている場合、サポートアングルはそのラックのメーカーが販売しているものをご使用ください。  
上下に隙間無く収納される場合は、サポートアングルにより取付かない場合がありますのでご確認のうえ取付けてください。

○ ラックマウントフレームと機器は、完全に固定されているわけではありません。機器をフレームに収納する際に、フレームを立てたり、横にしたり、逆さまにすると大変危険ですのでご注意ください。

#### 仕様

質量 RM-608J 約 5.2kg  
RM-608E 約 5.0kg

寸法(組立後)  
RM-608J 476(W)×149(H)×420(D)mm  
RM-608E 476(W)×133(H)×420(D)mm

# TEXIO

## INSTRUCTION MANUAL

### RACK MOUNT FRAME

# RM-608J/E

TEXIO TECHNOLOGY CORPORATION

© PRINTED IN JAPAN B71-0033-00

The RJ-608J/E is the standard rack mount frame in conformance to the JIS or EIA Standards. It is designed to mount our products.


Use the optional brackets to mount products suitable to them.

### 1. COMPONENT PARTS LIST

		Q'ty	Remark
①	Handle frame (R)	1	
②	Handle frame (L)	1	
③	Frame (shelf)	1	
④	Frame (upper)	1	* RM-608J only
⑤	Oval head screw	4	N33-5014-41
⑥	Angle washer	4	N19-0722-05
⑦	Flat head screw	10	N32-3006-41


### 3. INSTRUMENT MOUNTING PROCEDURES

- (1) Place an instrument ready to be mounted on the assembled rack mount frame. Slide the instrument backward until the projection at the back of the frame (shelf) ③ is inserted in the notch of the bracket fixed on the rear of the instrument. Then, fix the front bracket on the instrument to the frame (shelf) ③ with the Semmes screws. (Use the screws supplied with the bracket.)

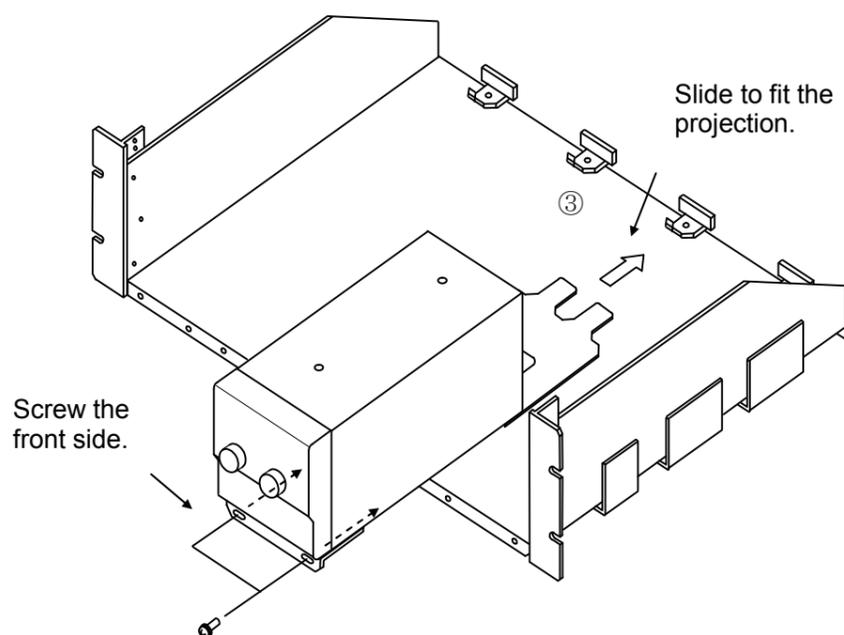

### INSTRUCTIONS


○The instrument is heavy. Attach support angles after mounting it on the rack.

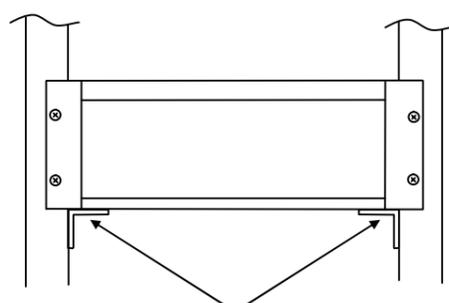

Support angles


We provide no support angles. Use support angles provided by the rack manufacturer, when a mass-marketed rack is used. If the instrument is mounted with no spaces above and below it, the support angles may not be attached. Check before mounting.

### 2. ASSEMBLY PROCEDURES OF RACK MOUNT FRAMES

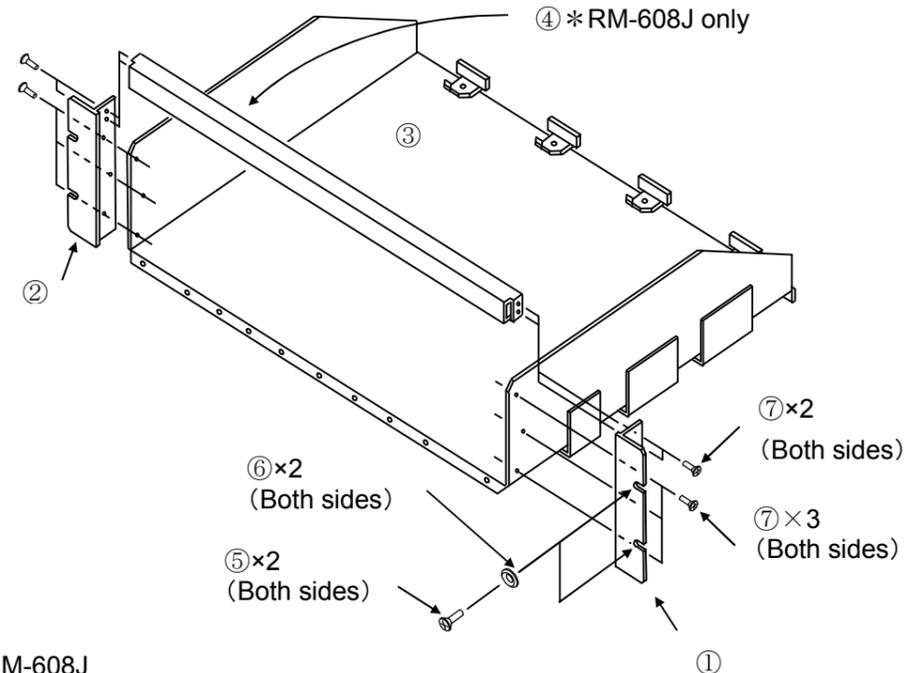

#### (2) RM-608J

- Place the frame (upper) ④ on the top of the fixed instrument. Fix it to the handle frames on both sides (R) and (L) with the flat head screws ⑦.

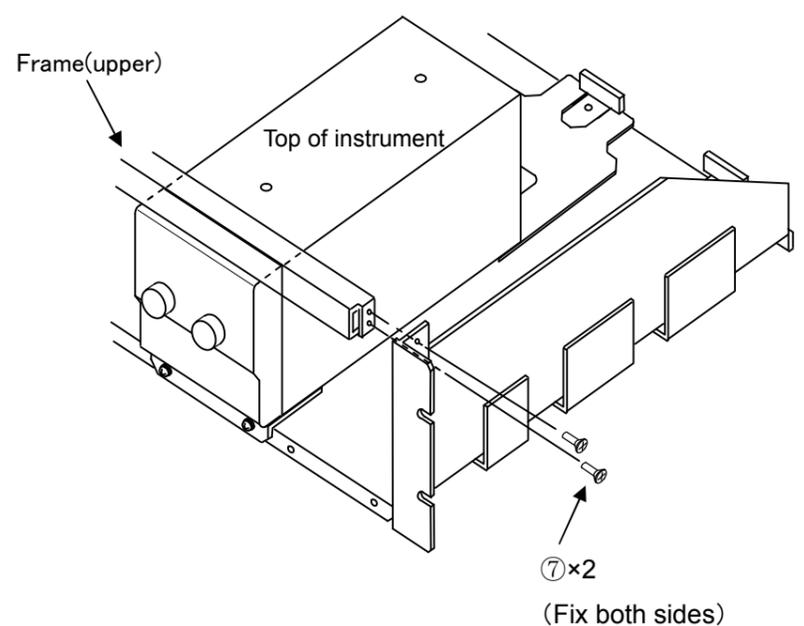

○The instrument is not fixed completely with the rack mount frame.

It is very dangerous to stand the frame, place it on its side or turn it upside down when mounting the instrument on the frame.

#### Specifications

Weight RM-608J: Approx. 5.2 kg  
RM-608E: Approx. 5.0 kg

#### Dimensions (after assembly)

RM-608J: 476 W x 149 H x 420 D mm  
RM-608E: 476 W x 133 H x 420 D mm